


1632 Oxygen Analyser Trouble Shooting Flowchart



**WARNING: Mains voltage terminals are exposed inside the analyser.
Only authorised personnel should work on this equipment.**

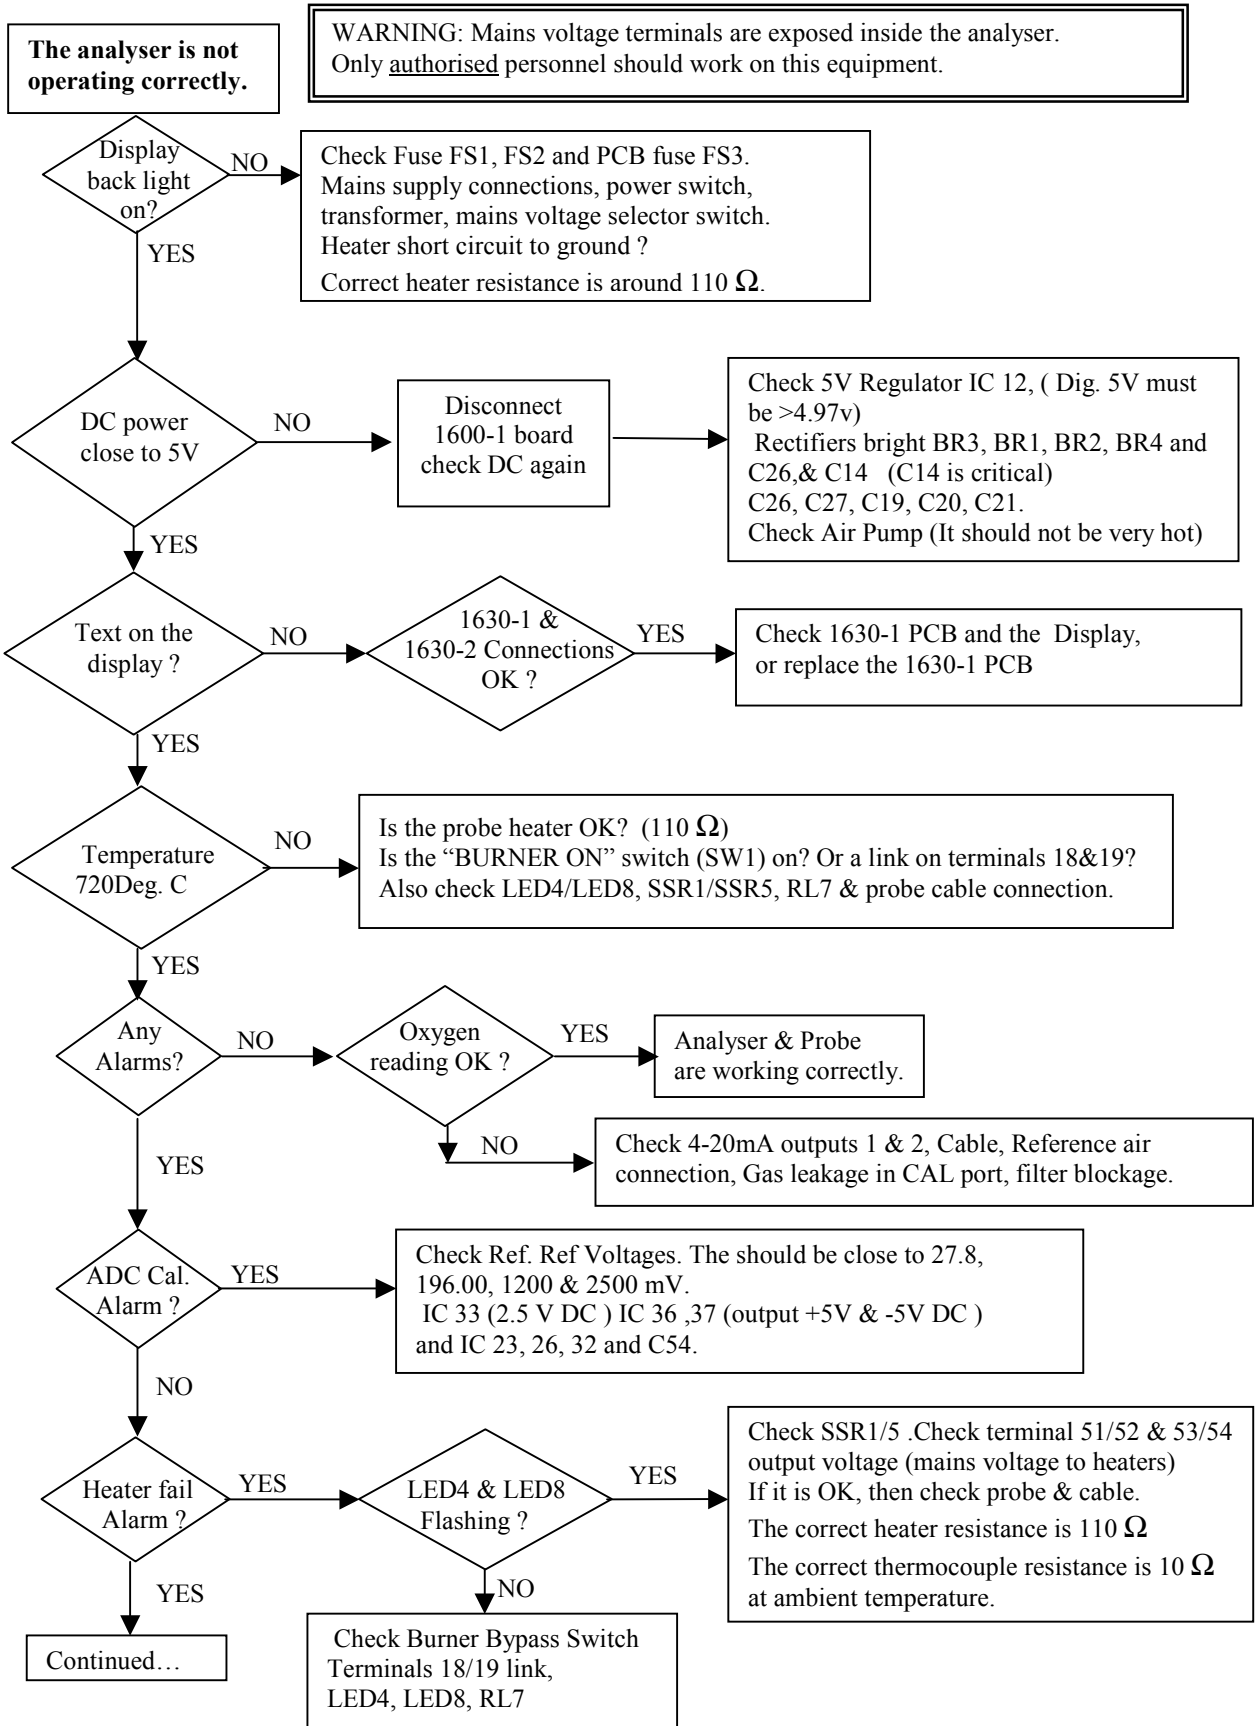